


# Blood Separation

## WHERE TO START

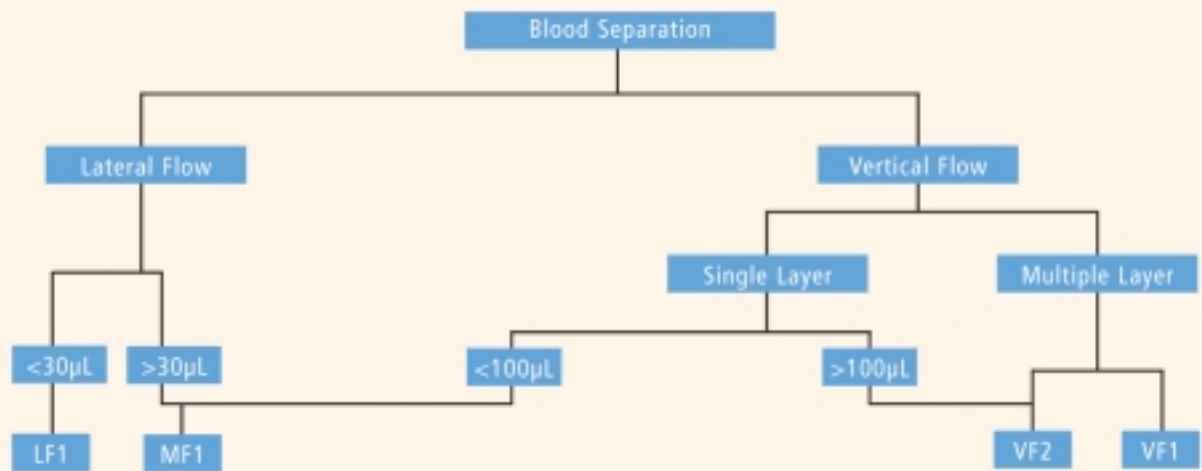

20.0	20.0	Minimum volume of whole blood that can be used (µL)	40.0	40.0
0.59	0.77	Minimum area of separator to separate the minimum volume (cm <sup>2</sup> )	0.47	0.52
21.2	17.6	Typical volume of serum recovered from 40µL of whole blood	14.4	16.1
86.0	73.0	Percentage of available serum obtained (%)	60.0	67.0
46.0	57.0	Basis weight (g/m <sup>2</sup> )	125.0	121.0
247.0	367.0	Thickness (µm@53kPa)	785.0	632.0